Prospera™

Sample Collection Instructions

Transplant assessment



DO NOT store kits in an area where the temperature range is outside 65°F-86°F



DO NOT expose **blood** to temperatures outside the range of 43°F-98°F (6°C-37°C).

1. Collect the patient's blood



10 mL of blood in each of two Streck cell-free DNA tubes

- Fill both tubes completely. If insufficient volume is obtained, please draw an additional tube.
- Allow 60–90 seconds for each tube to fill.
- Use a 21 gauge straight needle. **DO N** use a butterfly needle.
- Vein collapse may require a second venipuncture with a fresh tube.

2. Gently mix the sample









x 10

• Gently invert each tube at least 10 times immediately after draw in order to thoroughly mix blood with reagents.




- DO NOT shake vigorously.
- **DO NOT** seal tubes with paraffin film.

Prospera™

Transplant assessment

Sample Collection Instructions (Continued)

3. Pre-pack the sample

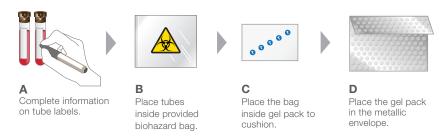

4. Ship the sample



This test was developed by Natera, Inc., a laboratory certified under the Clinical Laboratory Improvement Amendments (CLIA). This test has not been cleared or approved by the US Food and Drug Administration (FDA). Although FDA does not currently clear or approve laboratory-developed tests in the US, certification of the laboratory is required under CLIA to ensure the quality and validity of the tests. MLB-10096 Rev01 Prospera Domestic Sample Collection Instructions-NAT-801960 © 2019 Natera, Inc.



